


BOWIE DICK TEST PACK

Colour change 134 °C 3.5 Min.
Pink to Black 121°C 10 Min.

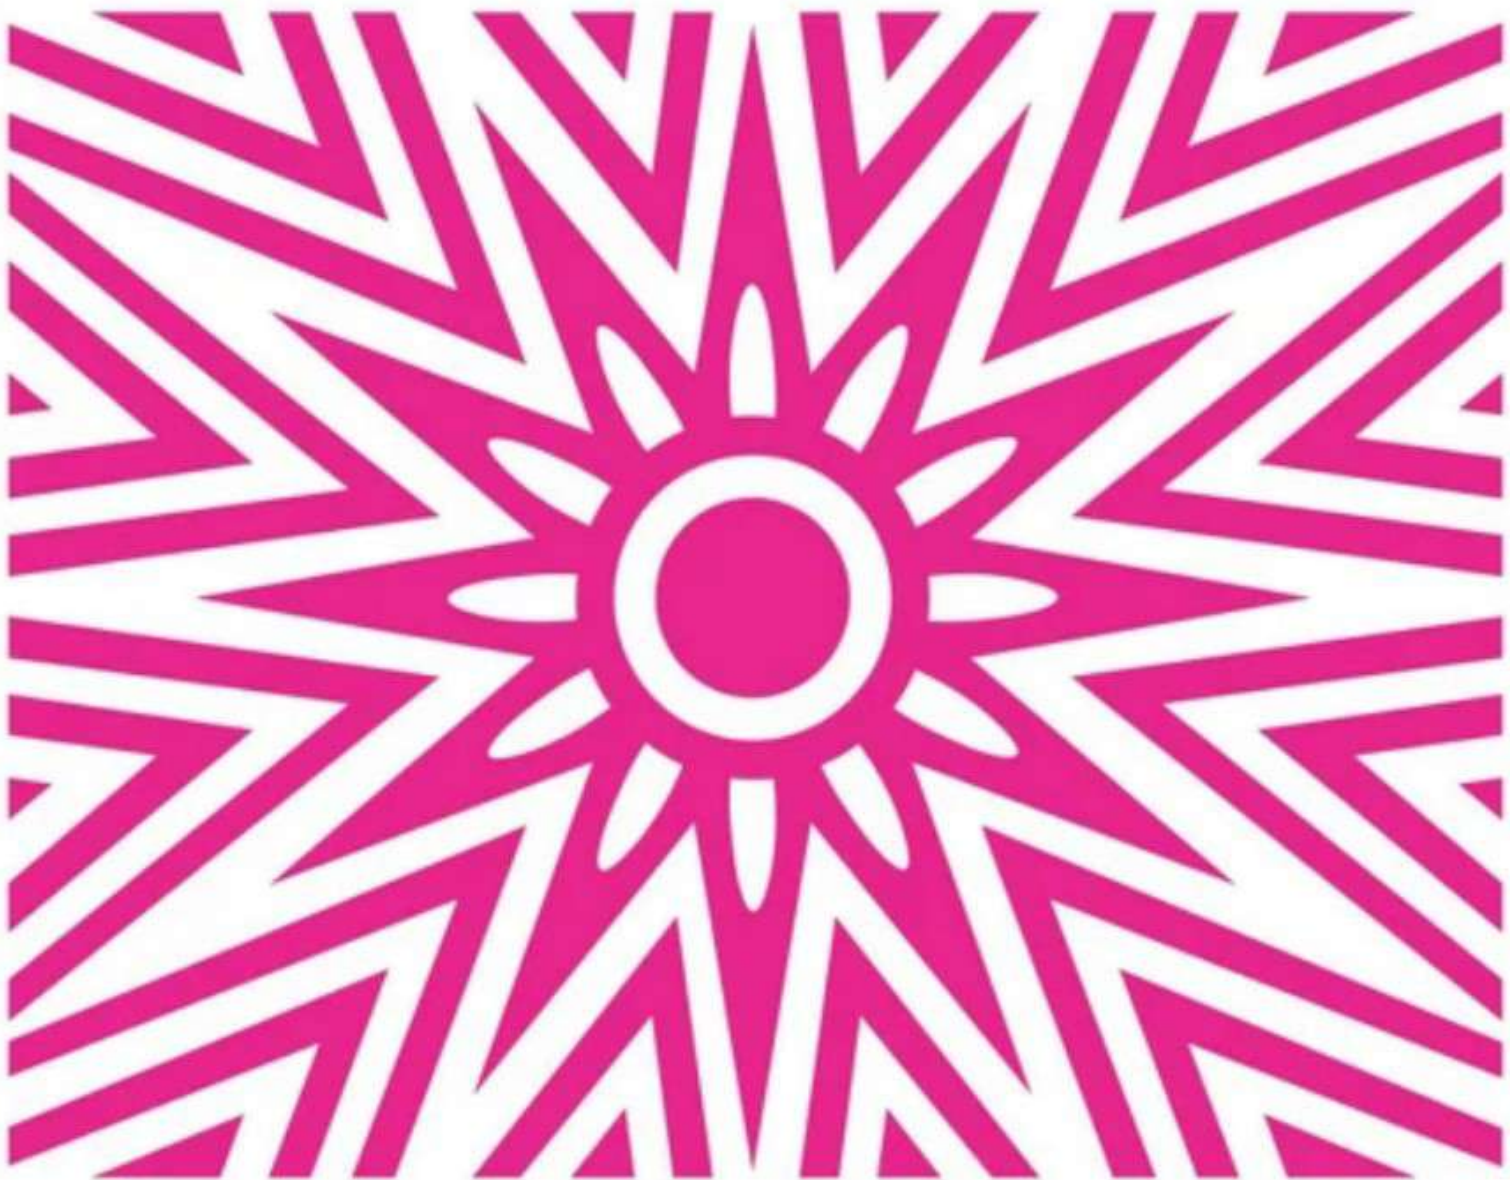

Date _____ Autoclave No. _____ Site _____ Cycle No. _____
Operator _____ Supervisor _____ Deptt. _____ Result _____
ISO 111440-1 CLASS 2 LOT RSM052024  05-2024  04-2027