



RIVERSIDE MEDICAL

Mfg. and Supply of all Medical CSSD Products


www.rsmmedical.com

A photograph showing a person wearing blue nitrile gloves handling several white, sealed sterilization pouches containing surgical instruments. The scene is set in a sterile environment, likely a sterilization department.

STERILIZATION DEPARTMENT


BOWIE DICK TEST PACK

BOWIE DICK TEST PACK Colour change Pink to Black 134 °C 3.5 Min. 121 °C 10 Min.

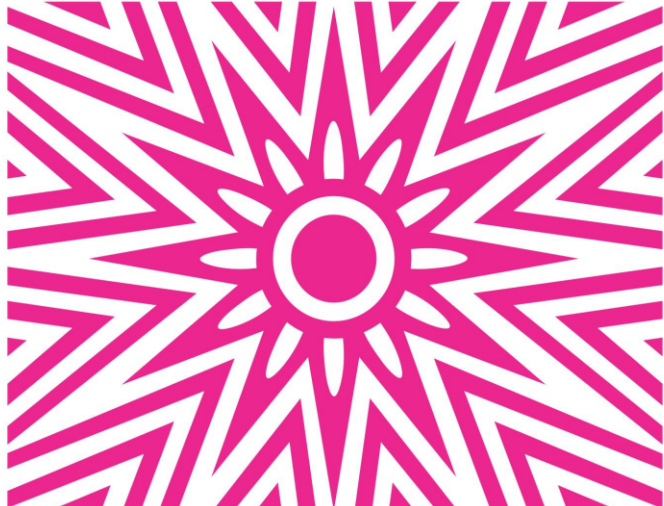

Date _____ Autoclave No. _____ Site _____ Cycle No. _____
 Operator _____ Supervisor _____ Deptt. _____ Result _____
 ISO 111440-1 CLASS 2 [LOT] RSM052024 [MFG] 05-2024 [EXP] 04-2027


RSM AIR REMOVAL STEAM 121°C 11 Min. Lead Free Indicator Ink

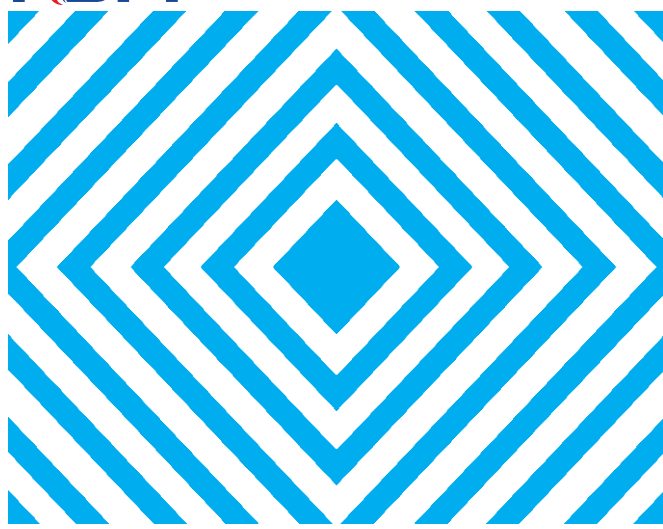

Hospital..... Department..... Autoclave No..... Cycle No.....
 Supervisor..... Operator..... Date..... Result.....
 ISO 11140-1 Class-2 LOT- W0425 Manu.- 022024 Exp.- 012026

STEAM & ETO CHEMICAL INDICATOR

RSM STEAM **Chemical Integrator**
 121°C 15 min 134°C 3.5 min
 EN ISO 11140-1 **CLASS 5**
 [LOT] RSM427 [REF] R-2831
 [MFG] 2024-04 [EXP] 2027-03 [RECYCLE] SELF ADHESIVE




Pink to Black

EO Type 5 **RSM**
ETHYLENE OXIDE INTEGRATOR
 EN ISO 11140-1 [RECYCLE] Self Adhesive
 BLUE TO GOLDEN YELLOW / BROWN [LOT] RSM0629 [MFG] 2024-12 [EXP] 2027-11




RSM STEAM **Chemical Integrator**
 121°C 15 min 134°C 3.5 min
 EN ISO 11140-1 **CLASS 5**
 [LOT] RSM427 [REF] R-2831
 [MFG] 2024-04 [EXP] 2027-03 [RECYCLE] SELF ADHESIVE




Blue to Black

Chemical Integrator STEAM **RSM**
 121°C 15 min 134°C 3.5 min
CLASS 4 EN ISO 11140-1
 [LOT] RSM427 [REF] R-2832
 [MFG] 2024-05 [EXP] 2028-04 [RECYCLE] SELF ADHESIVE Pink to Black




RSM STEAM Type 6 121°C 15 min 134°C 3.5 min
EMULATING INDICATOR
 EN ISO 11140-1 [RECYCLE]
 [LOT] RSO418 [REF] C-2810
 [MFG] 2023-07 [EXP] 2026-06 SELF ADHESIVE




Pink to Black


Chemical Integrator STEAM **RSM**
 121°C 15 min 134°C 3.5 min
CLASS 4 EN ISO 11140-1
 [LOT] RSM426 [REF] R-2831
 [MFG] 2024-03 [EXP] 2028-02 [RECYCLE] SELF ADHESIVE Green to Purple



RSM Type 6 STEAM **EMULATING INDICATOR**
 EN ISO 11140-1
 121°C 15 min 134°C 3.5 min
 [LOT] RSM50124 [MFG] 2024-12 [EXP] 2028-11 Pink to Black



RSM **EO** Blue to Golden Yellow/Brown
Ethylene Oxide Gas Integrator
 Type 4
 EN ISO 11140-1
 MFG Date : 062024
 Exp. Date : 052027
 Lot No. : RSM0625



A4 SIZE BOWIE DICK TEST SHEET

Autoclave No	BOWIE DICK TEST SHEET		Site		
	Cycle Number			Department	
					Date
					Supervisor
Operator					
Results					

STEAM
134° C - 3.5 MIN
121° C - 15 MIN

Bowie & Dick Test Sheet

ISO 11140-1 CLASS 2
ISO 11140-3
RSM 0627
0122024 112027

COLOUR CHANGE FROM BLUE TO BROWN / BLACK



Autoclave No	Bowie & Dick Test Sheet		Site		
	Cycle Number			Department	
					Date
					Supervisor
Operator					
Results					

STEAM
134° C - 3.5 MIN
121° C - 15 MIN

Bowie & Dick Test Sheet

ISO 11140-1 CLASS 2
ISO 11140-3
RSM 0420
082023 072025

COLOUR CHANGE FROM BLUE TO BLACK

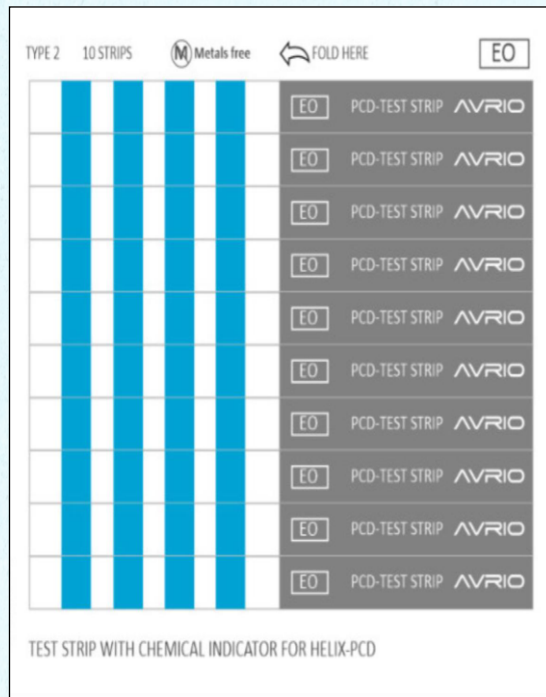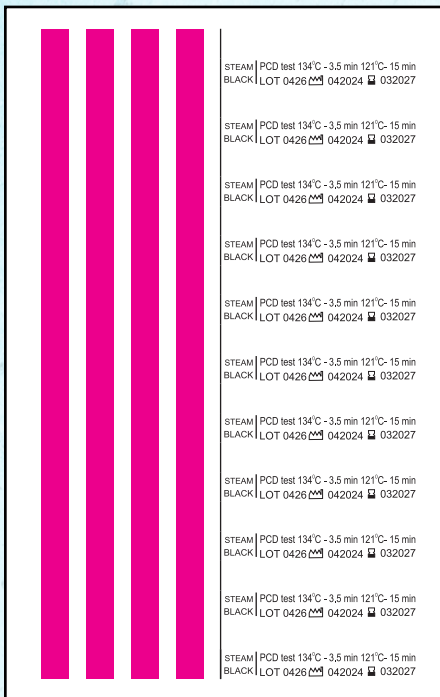

RSM




STEAM PENETRATION

RSM
CAT NO.: RSMP - 10

RSM

STEAM PENETRATION

RSM
CAT.NO.: RSMP - 10

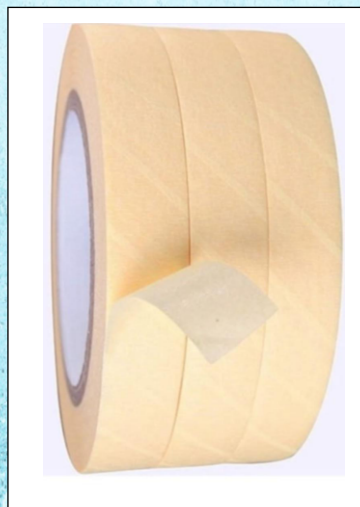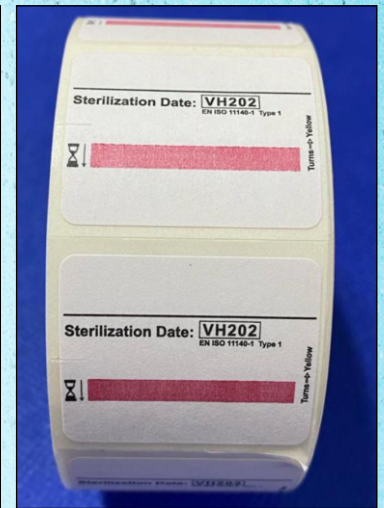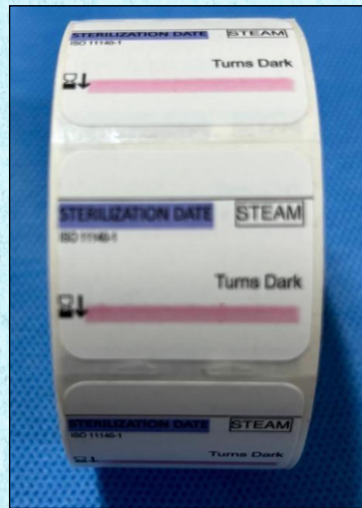

RIVERSIDE MEDICAL

C-445, Sobo Centre, Safal Parisar, Main Road, South Bopal, Ahmedabad - 380058
M.: 99136 20982 | 82384 72209 | E-mail: riverside2810@gmail.com | www.rsmmedical.com